

FIG. 3

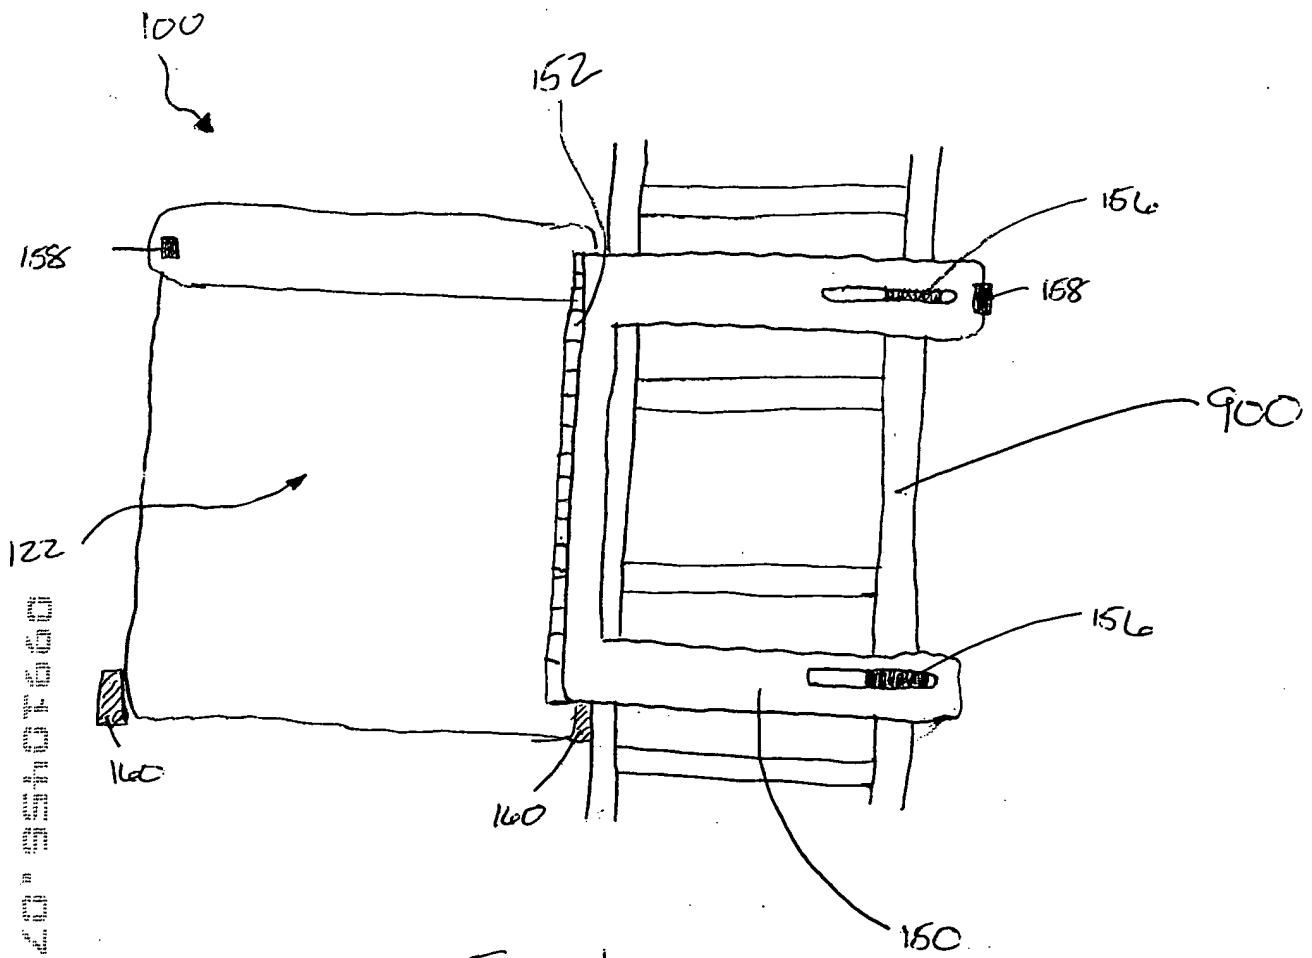


FIG. 4

FIG. 4

FIG. 5 is a perspective view of the device 500.

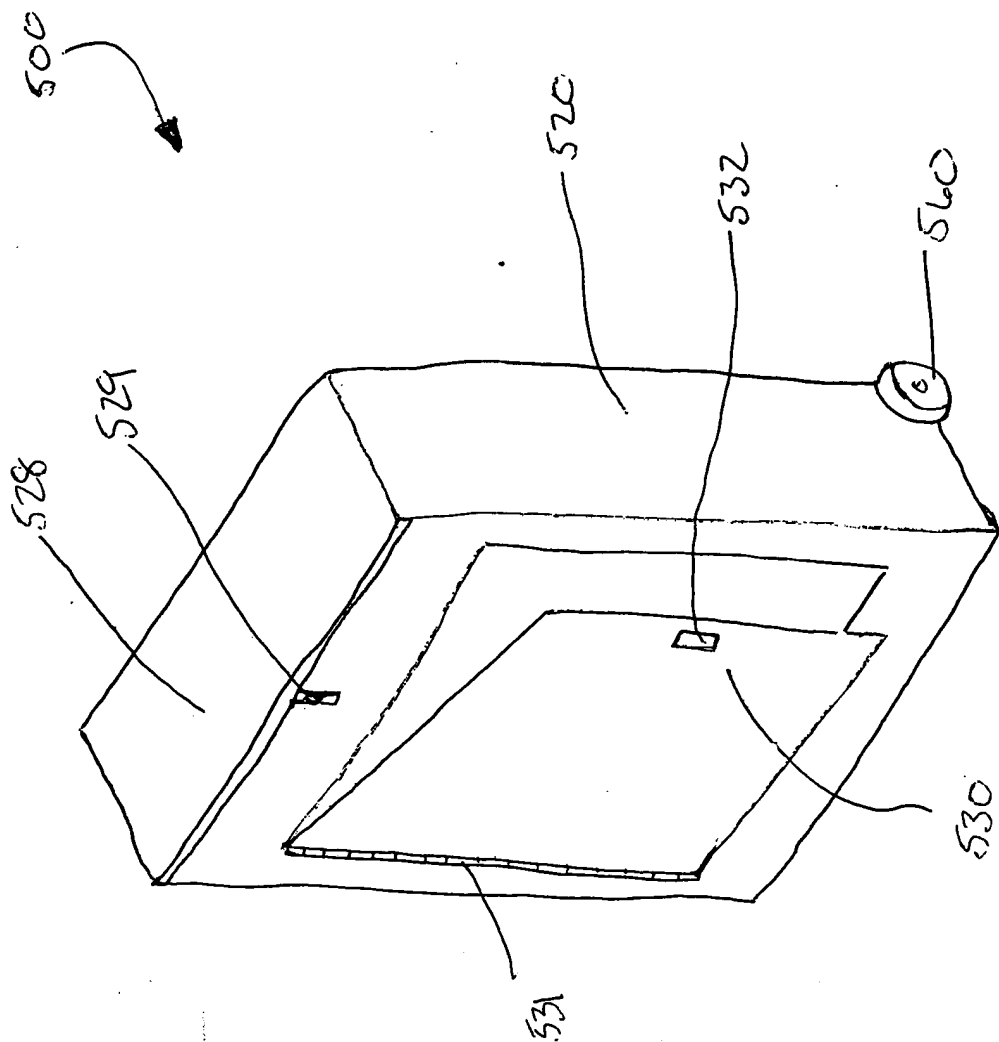


FIG. 5

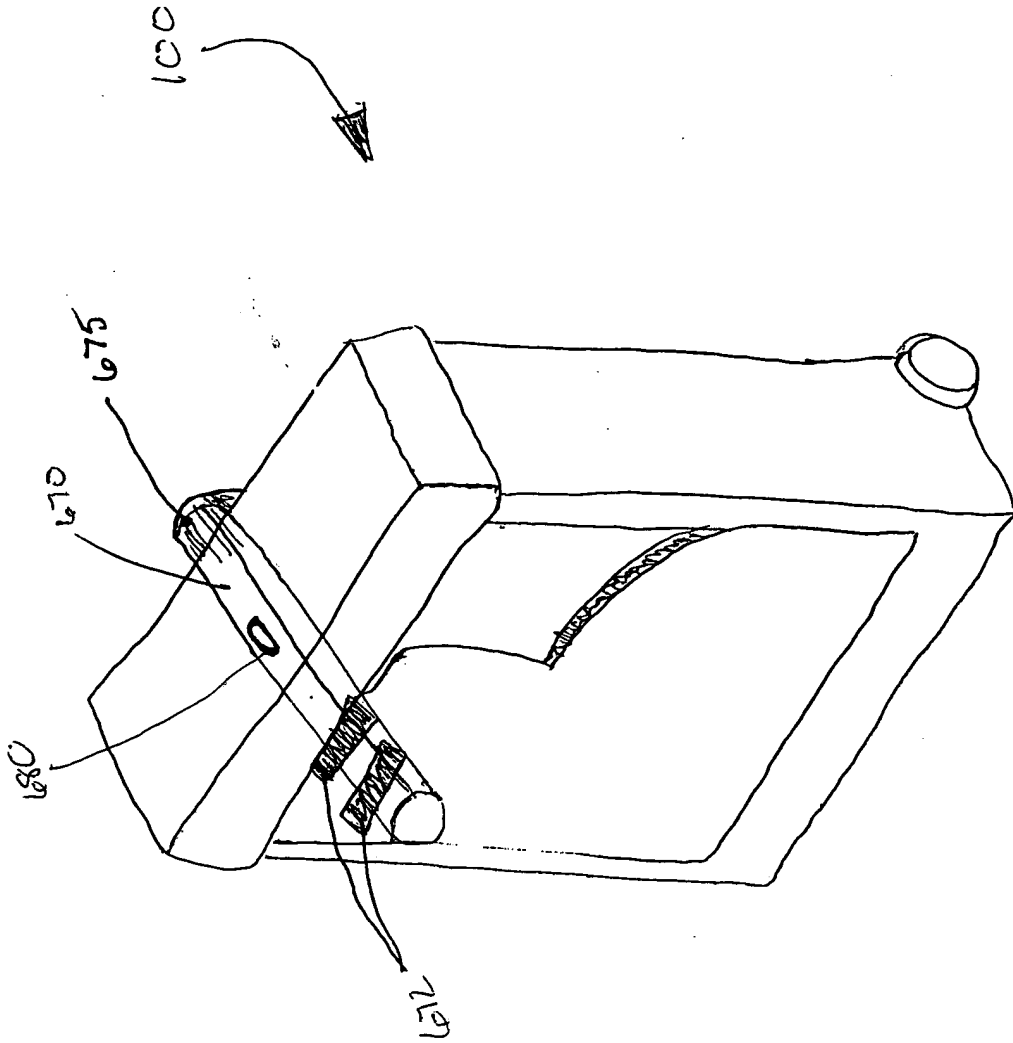


FIG. 6

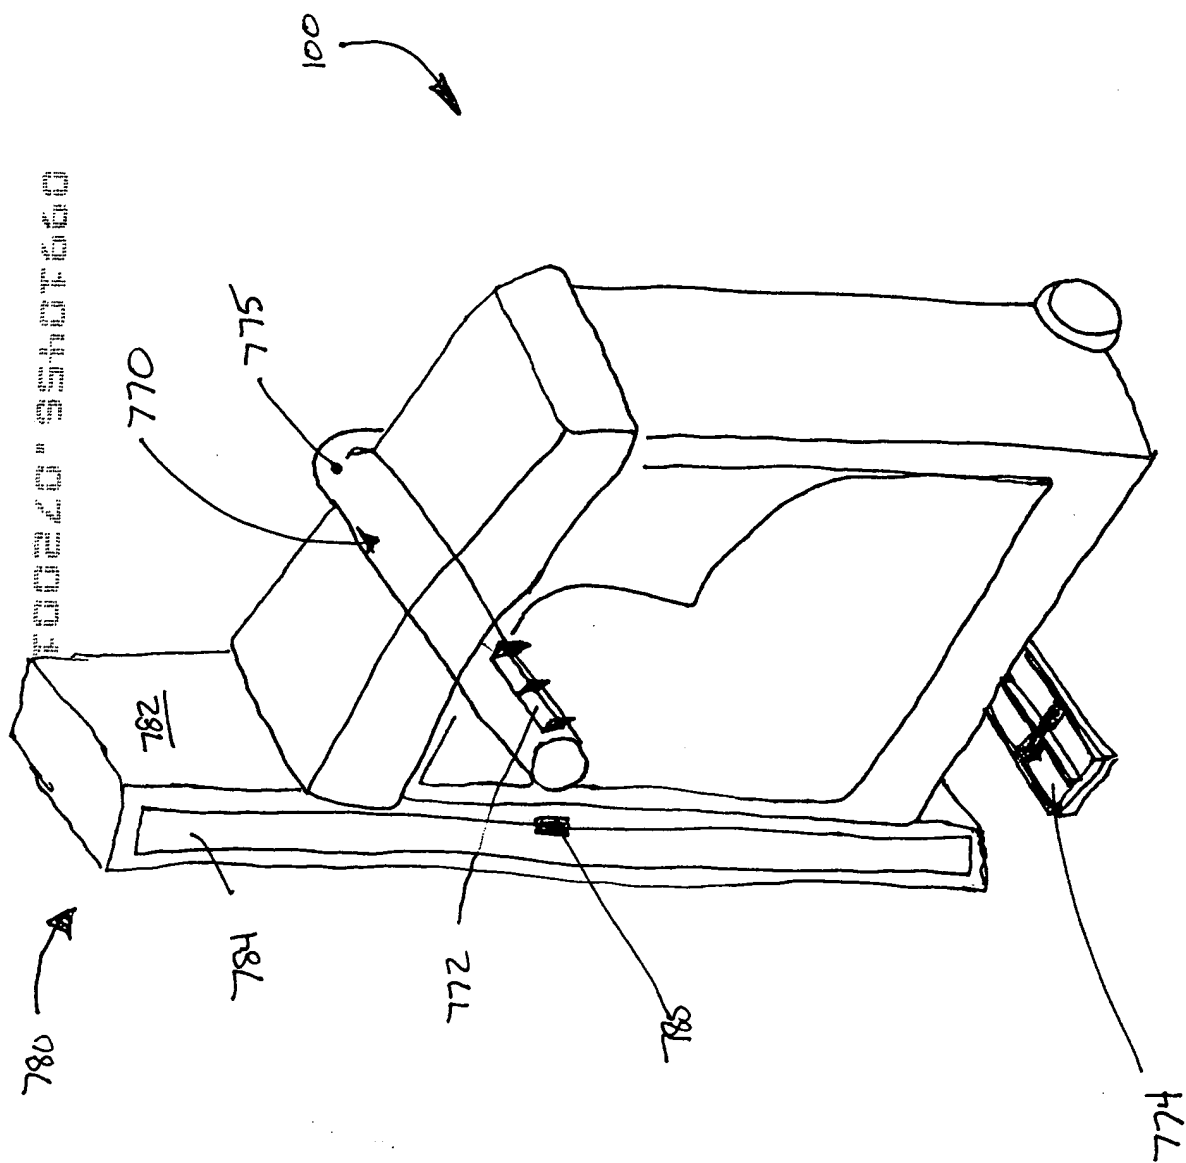


Fig. 7

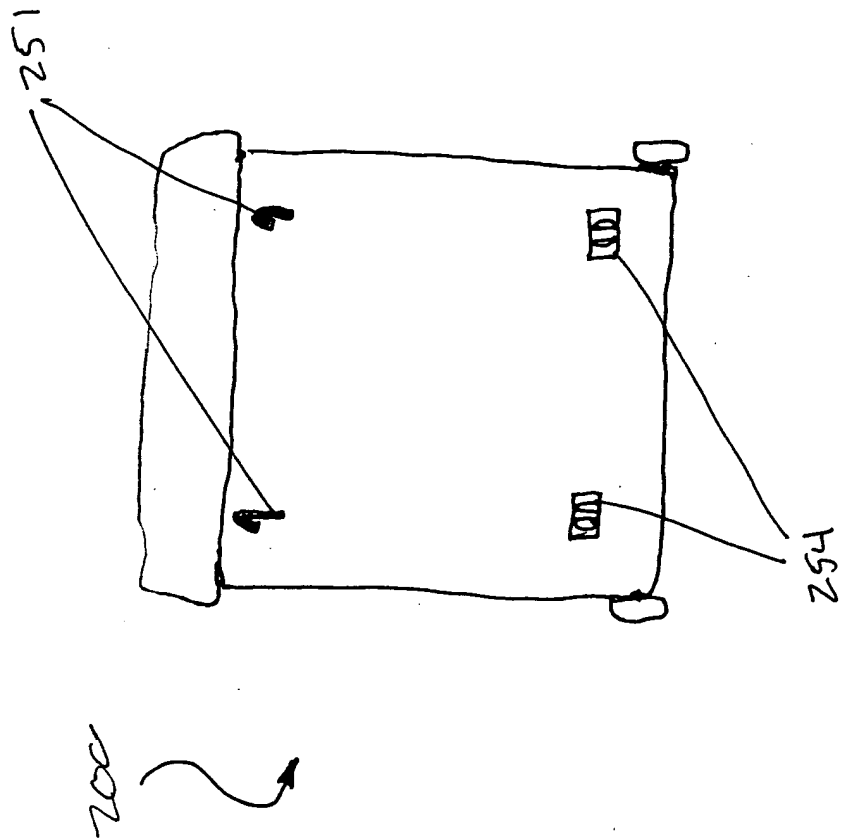


FIG. 8